

COURSE: Medical Microbiology, MBIM 650/720 - Fall 2009

TOPIC: Immunoglobulins: Ag-Ab Reactions and Selected Tests Lecture # 8

FACULTY: Dr. Haqqi  
Office: Bldg. #28, Rm 127  
Phone: 733-3216  
Email: Tariq.Haqqi@uscmed.sc.edu

TEACHING OBJECTIVES:

1. To describe the nature of Ag-Ab reactions
2. To compare and contrast antibody affinity and avidity
3. To delineate the basis for antibody specificity and cross reactivity
4. To discuss the principles of commonly used tests for antigen/antibody reactions

REQUIRED READING:

Male *et al.* Immunology, 7th Ed., pp 67-74


KEY WORDS:

Affinity, Avidity, Specificity, Cross reactivity, Agglutination, Hemagglutination, Agglutinin, Titer, Prozone, Passive hemagglutination, Direct Coomb's test, Indirect Coomb's test, Hemagglutination inhibition, Equivalence point, Antibody excess, Antigen excess, Radial immunodiffusion, Immunoelectrophoresis, Countercurrent immunoelectrophoresis, Radioimmunoassay, Enzyme linked immunosorbent assay, Competitive RIA/ELISA, Noncompetitive RIA/ELISA, Immunofluorescence, Flow cytometry, Complement fixation

IMMUNOGLOBULINS: AG-AB REACTIONS

I. NATURE OF AG-AB REACTIONS

- A. Lock and Key Concept - The combining site of an antibody is located in the Fab portion of the molecule and is constructed from the hypervariable regions of the heavy and light chains. X-Ray crystallography studies of antigens and antibodies interacting shows that the antigenic determinant nestles in a cleft formed by the combining site of the antibody as illustrated in Figure 1. Thus, our concept of Ag-Ab reactions is one of a key (i.e. the Ag) which fits into a lock (i.e. the Ab).

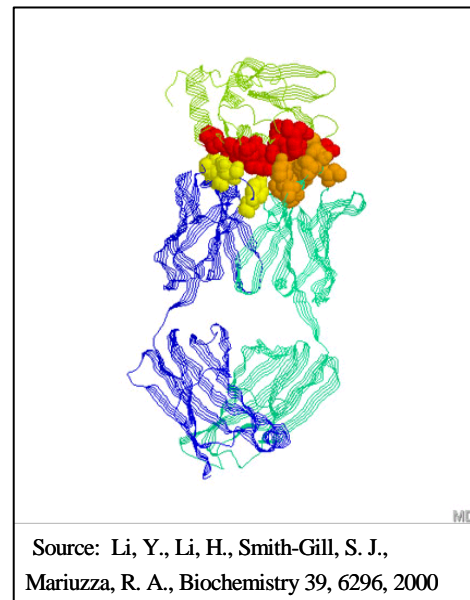

**Figure 1**

- B. **Non-covalent Bonds** - The bonds that hold the Ag in the antibody combining site are all non-covalent in nature. These include hydrogen bonds, electrostatic bonds, Van der Waals forces and hydrophobic bonds. Multiple bonding between the Ag and the Ab ensures that the Ag will be bound tightly to the Ab.
- C. **Reversible** - Since Ag-Ab reactions occur via non-covalent bonds they are by their nature reversible.

II. **AFFINITY AND AVIDITY**

A. **Affinity** - Antibody affinity is the strength of the reaction between a single antigenic determinant and a single combining site on the antibody. It is the sum of the attractive and repulsive forces operating between the antigenic determinant and the combining site of the antibody as illustrated in Figure 2.

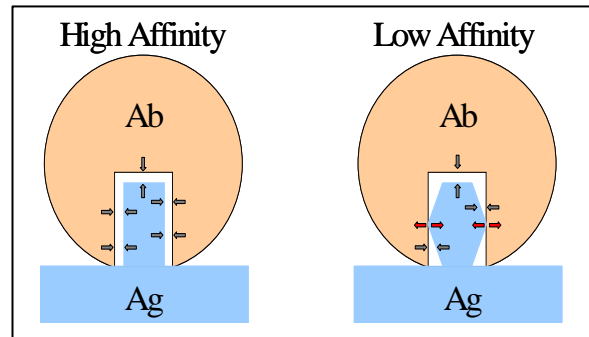


Figure 2

Affinity is the equilibrium constant that describes the Ag-Ab reaction as illustrated in Figure 3. Most antibodies have a high affinity for their antigens.

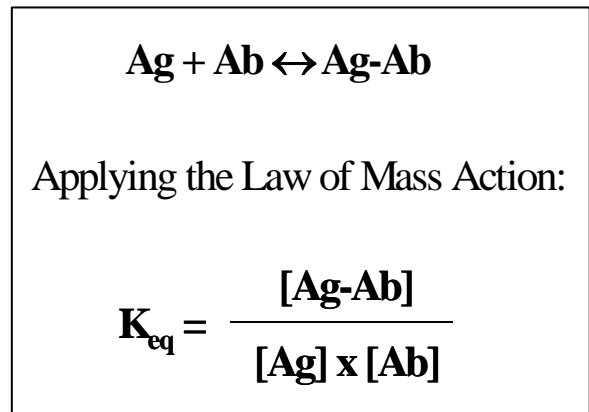


Figure 3

B. **Avidity** - Avidity is a measure of the overall strength of binding of an antigen with many antigenic determinants and multivalent antibodies. Affinity refers to the strength of binding between a single antigenic determinant and an individual antibody combining site whereas avidity refers to the overall strength of binding between multivalent Ag's and Ab's. Avidity is influenced by both the valence of the antibody and the valence of the antigen. Avidity is more than the sum of the individual affinities. This is illustrated in Figure 4.

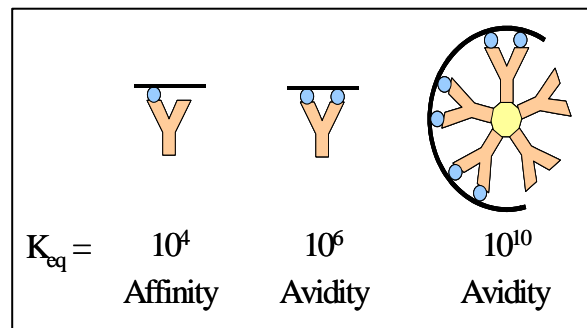


Figure 4

III. **SPECIFICITY AND CROSS REACTIVITY**

A. **Specificity** - Specificity refers to the ability of an individual antibody combining site to react with only one antigenic determinant or the ability of a population of antibody

molecules to react with only one antigen. In general, there is a high degree of specificity in Ag-Ab reactions. Antibodies can distinguish differences in 1) the primary structure of an antigen, 2) isomeric forms of an antigen, and 3) secondary and tertiary structure of an antigen.

B. **Cross reactivity** - Cross reactivity refers to the ability of an individual antibody combining site to react with more than one antigenic determinant or the ability of a population of antibody molecules to react with more than one antigen. Figure 5 illustrates how cross reactions can arise. Cross reactions arise because the cross reacting antigen shares an epitope in common with the immunizing antigen or because it has an epitope which is structurally similar to one on the immunizing antigen (multispecificity).

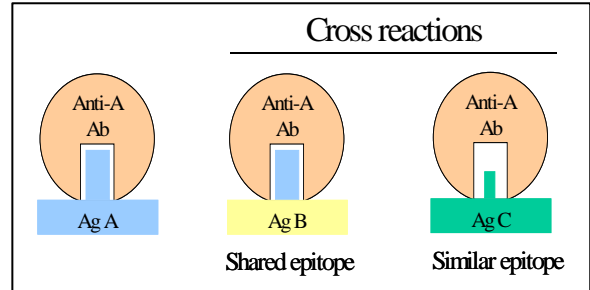


Figure 5

#### IV. TESTS FOR ANTIGEN-ANTIBODY REACTIONS

A. **Factors affecting measurement of Ag/Ab reactions** - The only way that one knows that an antigen-antibody reaction has occurred is to have some means of directly or indirectly detecting the complexes formed between the antigen and antibody. The ease with which one can detect antigen-antibody reactions will depend on a number of factors.

1. Affinity - The higher the affinity of the antibody for the antigen, the more stable will be the interaction. Thus, the ease with which one can detect the interaction is enhanced.

2. Avidity - Reactions between multivalent antigens and multivalent antibodies are more stable and thus easier to detect.

3. Ag:Ab ratio - The ratio between the antigen and antibody influences the detection of Ag/Ab complexes because the sizes of the complexes formed is related to the concentration of the antigen and antibody. This is depicted in Figure 6.

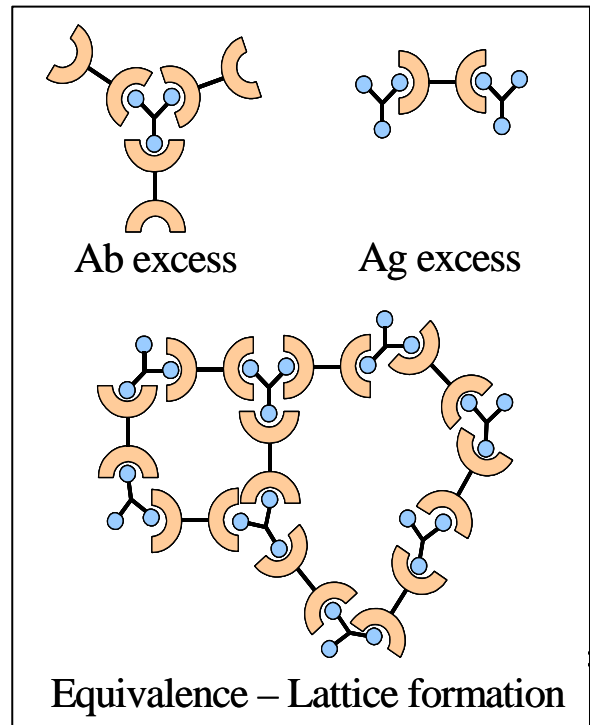



Figure 6

4. Physical form of the antigen - The physical form of the antigen influences how one detects its reaction with an antibody. If the antigen is a particulate, one generally looks for agglutination of the antigen by the antibody. If the antigen is soluble one generally looks for the precipitation of the antigen after the production of large insoluble Ag/Ab complexes.

**B. Agglutination Tests**

1. Agglutination/Hemagglutination - When the antigen is particulate the reaction of an antibody with the antigen can be detected by agglutination (clumping) of the antigen. When the antigen is an erythrocyte the term hemagglutination is used. The term agglutinin is used to describe antibodies that agglutinate particulate antigens. When the antigen is an erythrocyte the term hemagglutinin is often used. All antibodies can theoretically agglutinate particulate antigens but IgM due to its high valence is particularly good agglutinin and one sometimes infers that an antibody may be of the IgM class if it is a good agglutinating antibody.

a) **Qualitative agglutination test** - Agglutination tests can be used in a qualitative manner to assay for the presence of an antigen or an antibody. The antibody is mixed with the particulate antigen and a positive test is indicated by the agglutination of the particulate antigen. (Figure 7).

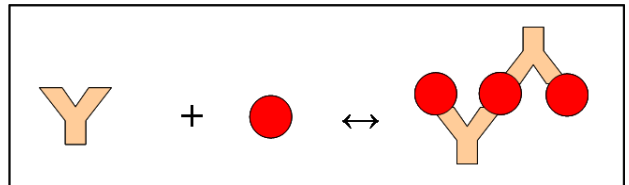

**Figure 7**

e.g. A patient's red blood cells mixed with antibody to a blood group antigen to determine a person's blood type.

e.g. A patient's serum mixed with red blood cells of known blood type to assay for the presence of antibodies to that blood type in the patient's serum.

b) **Quantitative agglutination test** - Agglutination tests can also be used to quantitate the level of antibodies to particulate antigens. In this test one makes serial dilutions of a sample to be tested for antibody and then adds a fixed number of red blood cells or bacteria or other such particulate antigen and determines the maximum dilution which gives agglutination. The maximum dilution that gives visible agglutination is called the **titer**. The results are reported as the reciprocal of the maximal dilution that gives visible agglutination. Figure 8 illustrates a quantitative hemagglutination test.

Patient	1/2	1/4	1/8	1/16	1/32	1/64	1/128	1/256	1/512	1/1024	Pos.	Neg.	Titer
1	●	●	●	●	●	●	●	●	●	●	●	●	64
2	●	●	●	○	○	○	○	○	○	○	●	○	8
3	●	●	●	●	●	●	●	●	●	●	●	○	512
4	○	○	●	●	●	●	●	●	●	●	●	○	<2
5	●	●	●	●	●	○	○	○	○	○	●	○	32
6	○	○	●	●	●	●	●	●	●	●	●	○	128
7	●	●	●	●	●	●	●	●	●	●	●	○	32
8	●	●	○	○	○	○	○	○	○	○	●	○	4

**Figure 8**

Prozone effect - On occasion one observes that when the concentration of antibody is high (i.e. lower dilutions) there is no agglutination and then as the sample is diluted agglutination occurs (See Patient 6 in Figure 8). The lack of agglutination at high concentrations of antibodies is called the prozone effect. Lack of agglutination in the prozone is due to antibody excess resulting in very small complexes which do not clump to form visible agglutination.

c) Applications of agglutination tests

1) Determination of blood types or antibodies to blood group antigens.

2) To assess bacterial infections

e.g. A rise in titer to a particular bacteria indicates an infection with that bacteria. N.B. a fourfold rise in titer is generally taken as a significant rise in antibody titer.

d) Practical considerations - Although the test is easy to perform, it is only semi-quantitative.

2. Passive hemagglutination - The agglutination test only works with particulate antigens. However, it is possible to coat erythrocytes with a soluble antigen (e.g. viral antigen, a polysaccharide or a hapten) and used the coated red blood cells in an agglutination test for antibody to the soluble antigen (Figure 9).

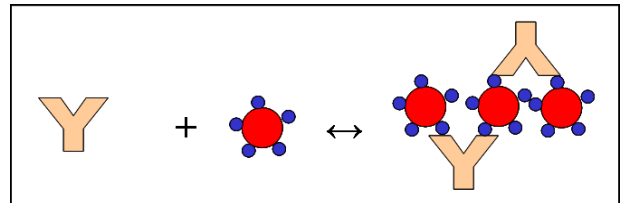



Figure 9

This is called passive hemagglutination. The test is performed just like the agglutination test. Applications include detection of antibodies to soluble antigens and detection of antibodies to viral antigens.

3. Coombs Test (Antiglobulin Test)

a) **Direct Coombs Test (Figure 10)** - When antibodies bind to erythrocytes, they do not always result in agglutination. This can result from the Ag/Ab ratio being


in antigen excess or antibody excess or in some cases electrical charges on the red blood cells preventing the effective cross linking of the cells. These antibodies that bind to but do not cause agglutination of red blood cells are sometimes referred to as incomplete antibodies. In no way is this meant to indicate that the antibodies are different in their structure, although this was once thought to be

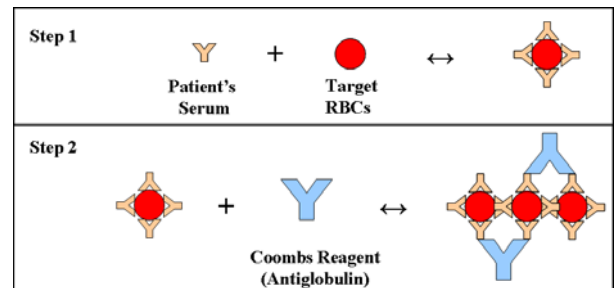

true. Rather it is functional definition only. In order to detect the presence of non-agglutinating antibodies on red blood cells, one simply adds a second antibody directed against the immunoglobulin (Ab) coating the red cells. This anti-immunoglobulin can now cross link the red blood cells and result in agglutination. This test is illustrated in Figure 10 and is known as the Direct Coombs test.

**b) Indirect Coombs Test (Figure 11)**


- If it is necessary to know whether a serum sample has antibodies directed against a particular red blood cell and you want to be sure that you also detect potential non agglutinating antibodies in the sample, an Indirect Coombs test is performed (Figure 11). This test is done by incubating the red blood cells with the serum sample, washing out any unbound antibodies and then adding a second anti-immunoglobulin reagent to cross link the cells.

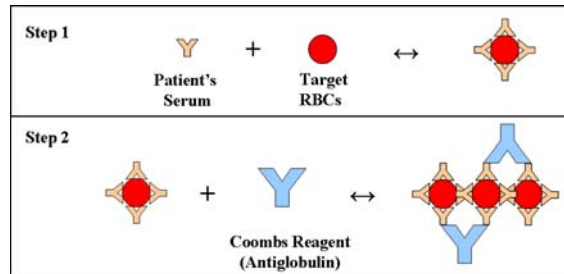

**Figure 11**

c) Applications include detection of anti-Rh antibodies. Antibodies to the Rh factor generally do not agglutinate red blood cells. Thus, red cells from Rh<sup>+</sup> children born to Rh<sup>-</sup> mothers, who have anti-Rh antibodies, may be coated with these antibodies. To check for this a direct Coombs test is performed. To see if the mother has anti-Rh antibodies in her serum an Indirect Coombs test is performed.

4. Hemagglutination Inhibition - The agglutination test can be modified to be used for the measurement of soluble antigens. This test is called hemagglutination inhibition. It is called hemagglutination inhibition because one measures the ability of soluble antigen to inhibit the agglutination of antigen-coated red blood cells by antibodies. In this test a fixed amount of antibodies to the antigen in question is mixed with a fixed amount of red blood cells coated with the antigen (see passive hemagglutination above). Also included in the mixture are different amounts of the sample to be analyzed for the presence of the antigen. If the sample contains the antigen, the soluble antigen will compete with the antigen coated on the RBC for binding to the antibodies, thereby inhibiting the agglutination of the RBC as illustrated in Figure 12.

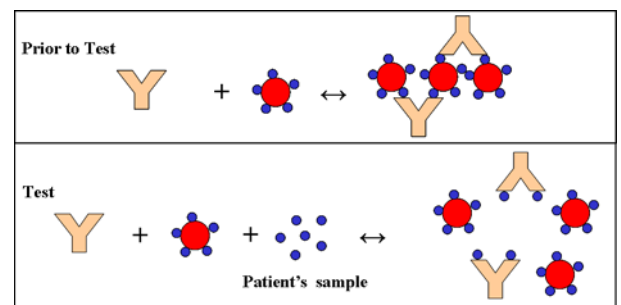

**Figure 12**

By serially diluting the sample, you can quantitate the amount of antigen in your unknown sample by its titer. This test is generally used to quantitate soluble

antigens and is subject to the same practical considerations as the agglutination test.

### C. Precipitation tests

1. **Radial Immunodiffusion (Mancini)** - In radial immunodiffusion antibody is incorporated into the agar gel as it is poured and different dilutions of the antigen are placed in holes punched into the agar. As the antigen diffuses into the gel it reacts with the antibody and when the equivalence point is reached a ring of precipitation is formed as illustrated in Figure 13.

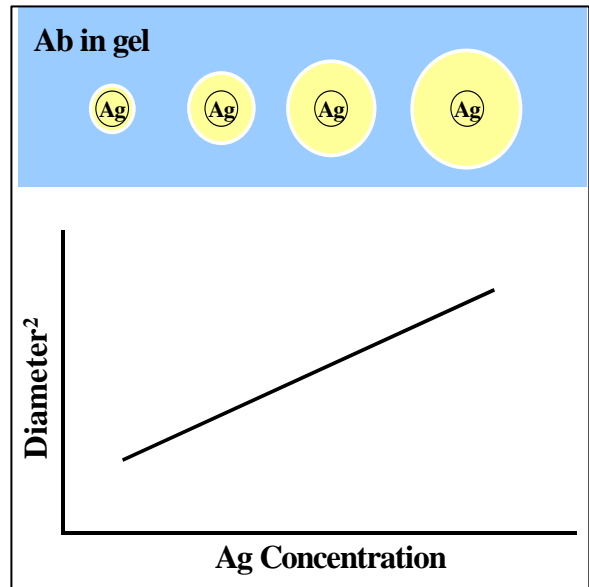


Figure 13

The diameter of the ring is proportional to the log of the concentration of antigen since the amount of antibody is constant. Thus, by running different concentrations of a standard antigen one can generate a standard curve from which one can quantitate the amount of an antigen in an unknown sample. Thus, this is a quantitative test. If more than one ring appears in the test, more than one antigen/antibody reaction has occurred. This could be due to a mixture of antigens or antibodies. This test is commonly used in the clinical laboratory for the determination of immunoglobulin levels in patient samples.

2. **Immuno-electrophoresis** - In immuno-electrophoresis a complex mixture of antigens is placed in a well punched out of an agar gel and the antigens are electrophoresed so that the antigen are separated according to their charge. After electrophoresis a trough is cut in the gel and antibodies are added. As the antibodies diffuse into the agar, precipitin lines are produced in the equivalence zone when an Ag/Ab reaction occurs as illustrated in Figure 14.

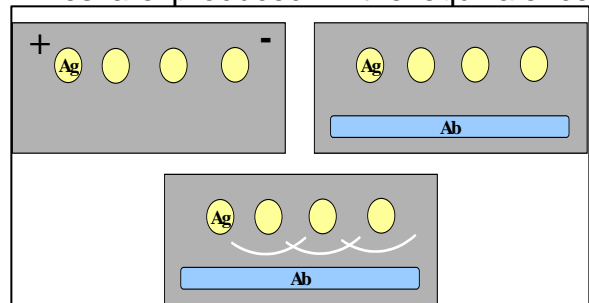


Figure 14

This test is used for the qualitative analysis of complex mixtures of antigens, although a crude measure of quantity (thickness of the line) can be obtained. This test is commonly used for the analysis of components in a patient's serum. Serum is placed in the well and antibody to whole serum in the trough. By comparisons to normal serum one can determine whether there are deficiencies on one or more serum components or whether there is an overabundance of some

serum component (thickness of the line). This test can also be used to evaluate purity of isolated serum proteins.

3. **Countercurrent electrophoresis** - In this test the antigen and antibody are placed in wells punched out of an agar gel and the antigen and antibody are electrophoresed into each other where they form a precipitation line as illustrated in Figure 15. This test only works if conditions can be found where the antigen and antibody have opposite charges. This test is primarily qualitative, although from the thickness of the band you can get some measure of quantity. It's major advantage is it's speed.

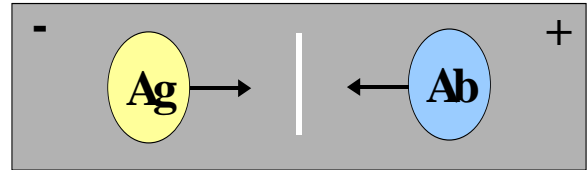


Figure 15

D. **Radioimmunoassay (RIA)/Enzyme Linked Immunosorbent Assay (ELISA)**

Radioimmunoassays (RIA) are assays which are based on the measurement of radioactivity associated with immune complexes. In any particular test, the label may be on either the antigen or the antibody. Enzyme Linked Immunosorbent assays (ELISA) are those that are based on the measurement of an enzymatic reaction associated with immune complexes. In any particular assay the enzyme may be linked to either the antigen or the antibody.

1. Competitive RIA/ELISA for Ag Detection -

The method and principle of RIA and ELISA for the measurement of antigen is shown in Figure 16. By using known amounts of a standard unlabeled antigen one can generate a standard curve relating cpm (Enzyme) bound vs amount of antigen. From this standard curve one can determine the amount of an antigen in an unknown sample.

The key to the assay is the separation of the immune complexes from the remainder of the components. This has been accomplished in many different ways and serves as the basis for the names given to the assay:

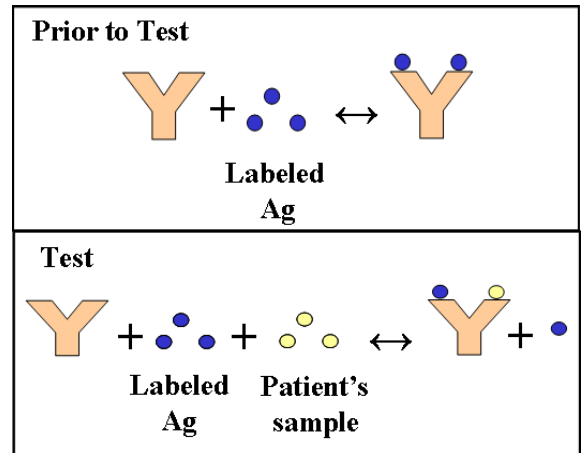


Figure 16

1) Precipitation with ammonium sulphate - Ammonium sulphate (33-50% final concentration) will precipitate immunoglobulins but not many antigen. Thus, this can be used to separate the immune complexes from free antigen. This has been called the Farr Technique

2) Anti-immunoglobulin antibody - The addition of a second antibody directed against the first antibody can result in the precipitation of the immune complexes and thus the separation of the complexes from free antigen.

3) Immobilization of the Antibody - The antibody can be immobilized onto the surface of a plastic bead or coated onto the surface of a plastic plate and thus the immune complexes can easily be separated from the other components by simply washing the beads or plate (Figure 17). This is the most common method used today and is referred to as Solid phase RIA or ELISA. In the clinical laboratory competitive RIA and ELISA are commonly used to quantitate serum proteins, hormones, drugs metabolites.

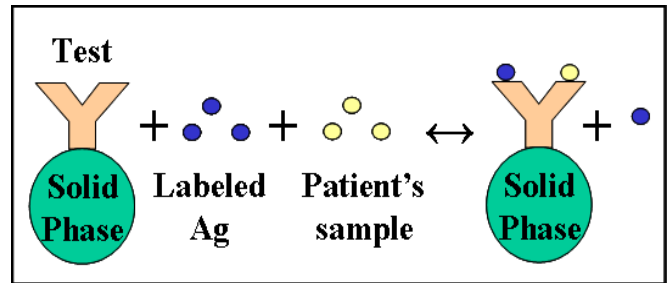


Figure 17

2. Noncompetitive RIA/ELISA for Ag or Ab - Noncompetitive RIA and ELISAs are also used for the measurement of antigens and antibodies. In Figure 18 the bead is coated with the antigen and is used for the detection of antibody in the unknown sample. The amount of labeled second antibody bound is related to the amount of antibody in the unknown sample. This assay is commonly employed for the measurement of antibodies of the IgE class directed against particular allergens by using a known allergen as antigen and anti-IgE antibodies as the labeled reagent. It is called the RAST test (radioallergosorbent test). In Figure 19 the bead is coated with antibody and is used to measure an unknown antigen. The amount of labeled second antibody that binds is proportional to the amount of antigen that bound to the first antibody.

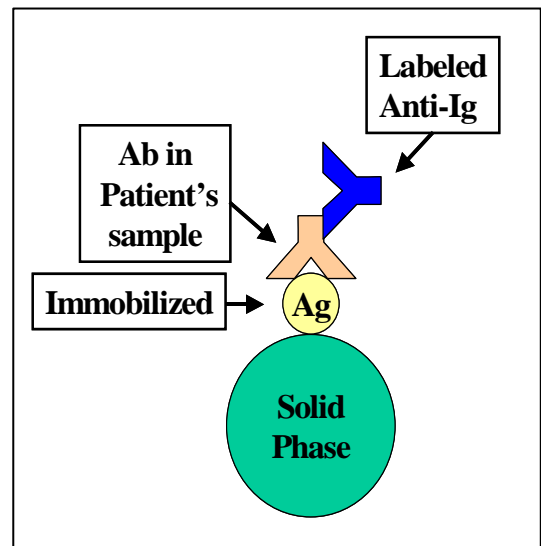


Figure 18

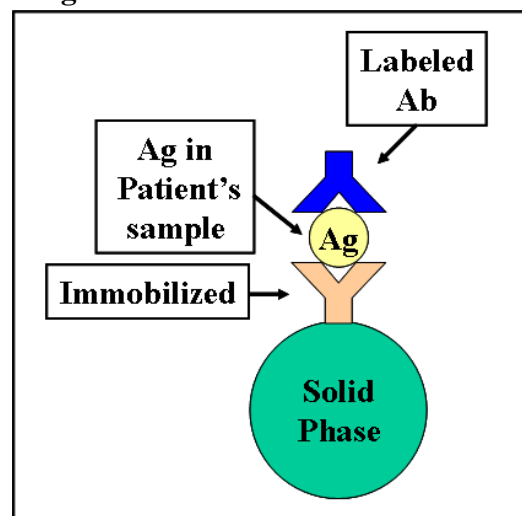


Figure 19

## F. Tests for Cell Associated Antigens

1. Immunofluorescence - Immunofluorescence is a technique whereby an antibody labeled with a fluorescent molecule (fluorescein or rhodamine) is used to detect the presence of an antigen in or on a cell or tissue by the fluorescence emitted by the bound antibody.

a) **Direct Immunofluorescence** - In direct immunofluorescence the antibody specific to the antigen is directly tagged with the fluorochrome (Figure 20).

b) **Indirect Immunofluorescence** - In indirect immunofluorescence the antibody specific for the antigen is unlabeled and a second anti-immunoglobulin antibody directed toward the first antibody is tagged with the fluorochrome (Figure 21). Indirect fluorescence is more sensitive than direct immunofluorescence since there is amplification of the signal.

c) **Flow Cytometry** - Flow cytometry is commonly used in the clinical laboratory to identify and enumerate cells bearing a particular antigen. Cells in suspension are labeled with a fluorescent tag by either direct or indirect immunofluorescence. The cells are then analyzed on the flow cytometer.

Figure 22 illustrates the principle of flow cytometry. In a flow cytometer the cells exit a flow cell and are illuminated with a laser beam. The amount of laser light that is scattered off the cells as they pass through the laser can be measured, which gives information concerning the size of the cells. In addition, the laser can excite the fluorochrome on the cells and the fluorescent light emitted by the cells can be measured by one or more detectors.

The type of data that is obtained from the flow cytometer is shown in Figure 23. In a one parameter histogram, increasing amounts of fluorescence (e.g. green fluorescence) is plotted on the x axis and the number of cells exhibiting that amount of fluorescence is plotted on the y axis. The fraction of cells that are fluorescent

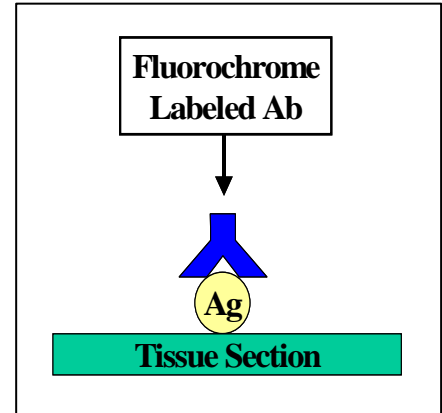


Figure 20

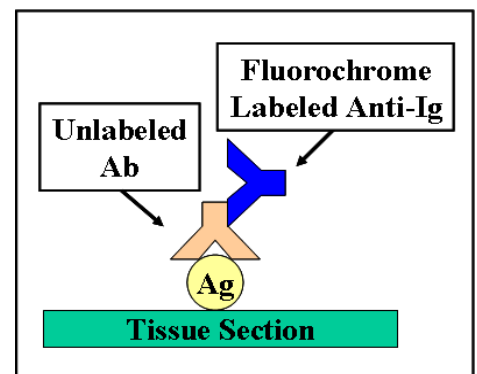


Figure 21

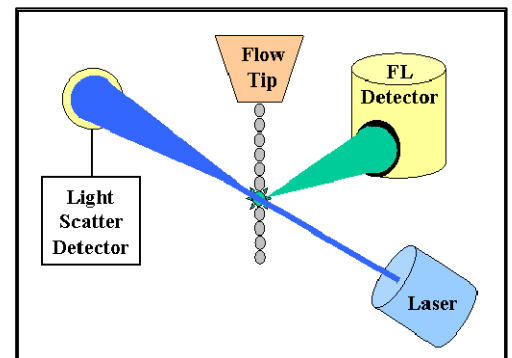


Figure 22

can be determined by integrating the area under the curve. In a two parameter histogram the x axis is one parameter (e.g. red fluorescence) and the y axis is the second parameter (e.g. green fluorescence). The number of cells is indicated by the contour and the intensity of the color.

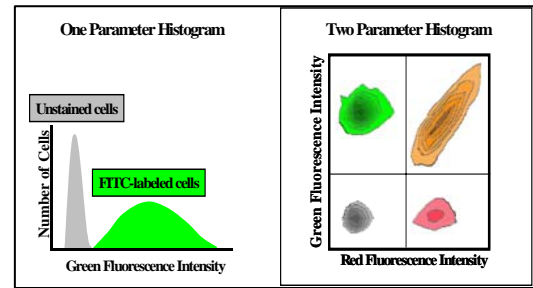


Figure 23

G. **Complement Fixation**

Antigen/Antibody complexes can also be measured by their ability to fix complement because an Ag/Ab complex will "consume" complement if it is present whereas free Ag's or Ab's do not. Tests for Ag/Ab complexes that rely on the consumption of complement are termed complement fixation tests and are used to quantitate Ag/Ab reactions. This test will only work with complement fixing antibodies (IgG, IgM best).

The principle of the complement fixation test is illustrated in Figure 24. Antigen is mixed with the test serum to be assayed for antibody and Ag/Ab complexes are allowed to form. A control tube in which no Ag is added is also prepared. If no Ag/Ab complexes are present in the tube, none of the complement will be fixed. However, if Ag/Ab complexes are present, they will fix complement and thereby reduce the amount of complement in the tube. After allowing for complement fixation by any Ag/Ab complexes, a standard amount of red blood cells, which have been pre-coated with anti-erythrocyte antibodies is added. The amount of antibody-coated RBC is predetermine to be just enough to completely use up all the complement initially added if it were still there. If all the complement was still present (i.e. no Ag/Ab complexes formed between the Ag and Ab in question), all the RBC will be lysed. If Ag/Ab complexes are formed between that Ag and Ab in question, some of the complement will be consumed and thus when the antibody-coated RBC's are added not all of them will lyse. By simply measuring the amount of RBC lysis by measuring the release of hemoglobin into the medium, one can indirectly quantitate Ag/Ab complexes in the tube. Complement fixation tests are most commonly used to assay for antibody in a test sample but they can be modified to measure antigen.

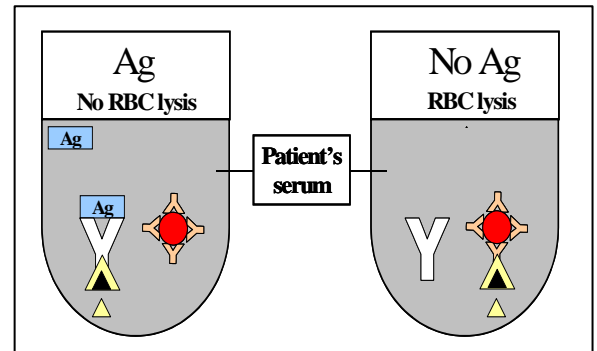


Figure 24

*Adapted from Dr. E.P.Mayer*